

Integration of Smart Infusion Pumps with Electronic Medical Record Reduces Potentially Catastrophic Medication Dosing Errors

King V., MS, BSN, Hum D., RPh, Kendzierski D., PharmD, Arvelo C., MBA, BSN, Overdyk F.J., MSEE, MD

Abstract

BACKGROUND

'Smart' infusion pumps with built-in dose error reduction software (DERS) containing hard and soft limits on prescribing ranges have, in retrospect, been found to eliminate only some of the medication errors associated with intravenous infusion.¹

In order to optimize "five rights" compliance, a greater level of smart pump integration enabling error checking and redundancy at all the contact points in the workflow is required.

Intravenous automated programming (IVAP) that enables the physician order, medication, and patient to be verified via barcode scanning at the point of care requires clinical integration of infusion devices with the EMR (CIDER).

OBJECTIVE

The purpose of this study was to determine the impact of CIDER on reducing serious, preventable medication errors, as classified by The National Coordinating Council for Medication Error Reporting and Prevention (NCC MERP) Medication Error Index. Furthermore, we were interested in the impact of CIDER in increasing drug library compliance and reducing variability of practice in programming infusion pumps.

CASE STUDY

From January 2013 to February 2014, there were 512,636 programming sequences recorded across three hospitals, 224,763 (44%) during the pre-integration period and 287,873 (56%) during the post-integration period.

CONCLUSION²

The incidence of potentially catastrophic dosing errors (PCDEs) across the combined group of three hospitals decreased after CIDER by 52%, from 7.1 errors per 1000 programs to 3.3 per 1000 programs, $P < 0.001$ (Table 1). Increase in compliance with drug library was 156% between the pre- and post-integration periods for the combined group of three hospitals from 20% to 51%, $P < 0.001$ (Table 2). Analysis over time shows a clear pivot in both results corresponding to CIDER "go-live" and is sustained after integration. Variability in the severity of individual PCDEs also displayed a large and statistically significant reduction.

All three of these metrics improved at each hospital.



Introduction

Medication errors associated with intravenous infusion remain a serious threat to patient safety in spite of numerous interventions to reduce their incidence. In order to ensure patients receive the right drug in the correct dose by the intended route for the appropriate period of time, a greater level of integration of the infusion device with its environment is needed.

Safer infusion therapy demands error checking and redundancy at all the contact points in the workflow, starting with the physician's order in the electronic medical record (EMR) to the pharmacy where the drug is compounded, converging at the point of care where the provider administers the drug via the device.

'Smart' infusion pumps with built-in dose error reduction software (DERS) containing hard and soft limits on prescribing ranges have, in retrospect, been found to eliminate only some of the medication errors.¹

Intravenous automated programming (IVAP) allows the physician order, medication, and patient to be verified via barcode scanning at the point of care and requires clinical integration of infusion devices with the EMR (CIDER).

Although CIDER can be initially complex and requires resources to support, healthcare facilities agree that it improves patient safety by eliminating the potential for human error and encourages drug library compliance, the use of barcode medication administration (BCMA) systems, and the standardization of nurse workflows.³ In this study, our primary outcome of interest was the impact of CIDER on reducing serious, preventable medication errors, as classified by The National Coordinating Council for Medication Error Reporting and Prevention (NCC MERP) Medication Error Index.⁴

Furthermore, we were interested in the impact of CIDER in increasing drug library compliance and reducing variability of practice in programming infusion pumps.

Methods



This study took place at three community hospitals with approximately 50, 150, and 350 beds where a Cerner Millennium® EMR was integrated with ICU Medical Plum A+® infusion pumps (Model #20792, ICU Medical MedNet® safety software rev 5.81) from January 1, 2013 to February 1, 2014 and was restricted to the following clinical areas: Cardiovascular ICU, ICU, Neuro Critical Care, MedSurg, Obstetrics, Oncology, and Progressive Care Unit (PCU).

We retrospectively analyzed infusion pump programming records before and after integration of infusion pumps with the EMR to measure the impact of CIDER on the incidence of PCDEs. We defined PCDEs as initial programmed doses/rates of intravenous medications considered ‘high alert’ medications⁵ by the Institute of Safe Medication Practices (ISMP) that were either 100% greater than or 50% less than the final programmed doses/rates. We hypothesized that these errors were likely to cause patient harm or require medical intervention to preclude harm if undetected. As such, the NCC MERP Medication Error Index would classify these events as ‘D’ through ‘I’.⁴ As a secondary outcome, we chose to measure pre- and post-integration compliance with the use of the drug library (as an opt-in step) when programming the Plum A+ infusion pump. ICU Medical MedNet safety software includes a drug library, which was custom-built for each clinical care area (CCA) and standardized as a single drug library across all three of the hospitals studied. Use of a DERS has been shown to reduce medication errors and improve patient safety.⁶ If the provider did not choose to opt in to ICU Medical MedNet when manually programming the Plum A+, that action was deemed noncompliant.

The workflow during the study was as follows. During the pre-integration period, the provider retrieved the physician’s medication order from the electronic medication administration record (eMAR) and programmed the infusion pump manually, including patient weight, drug, dose, rate, and volume to be infused at the point of care. Compliance with ICU Medical MedNet safety software was counted when the provider selected a medication from the drug list for that infusion. Subsequent programs for that infusion, such as titrations, were also counted as compliant with ICU Medical MedNet. If the provider bypassed the drug list, that infusion and subsequent titrations would be noncompliant with ICU Medical MedNet.

Post-integration, the provider ensures the “five rights” verification (right patient, medication, dose, time, and route) by signing into the eMAR, and by scanning the barcode on the patient, medication, and appropriate pump channel (primary or secondary). The completed order is displayed on the pump and the provider confirms and starts the infusion. (Figure 1).



Smart Pump-EMR Integration Workflow Overview

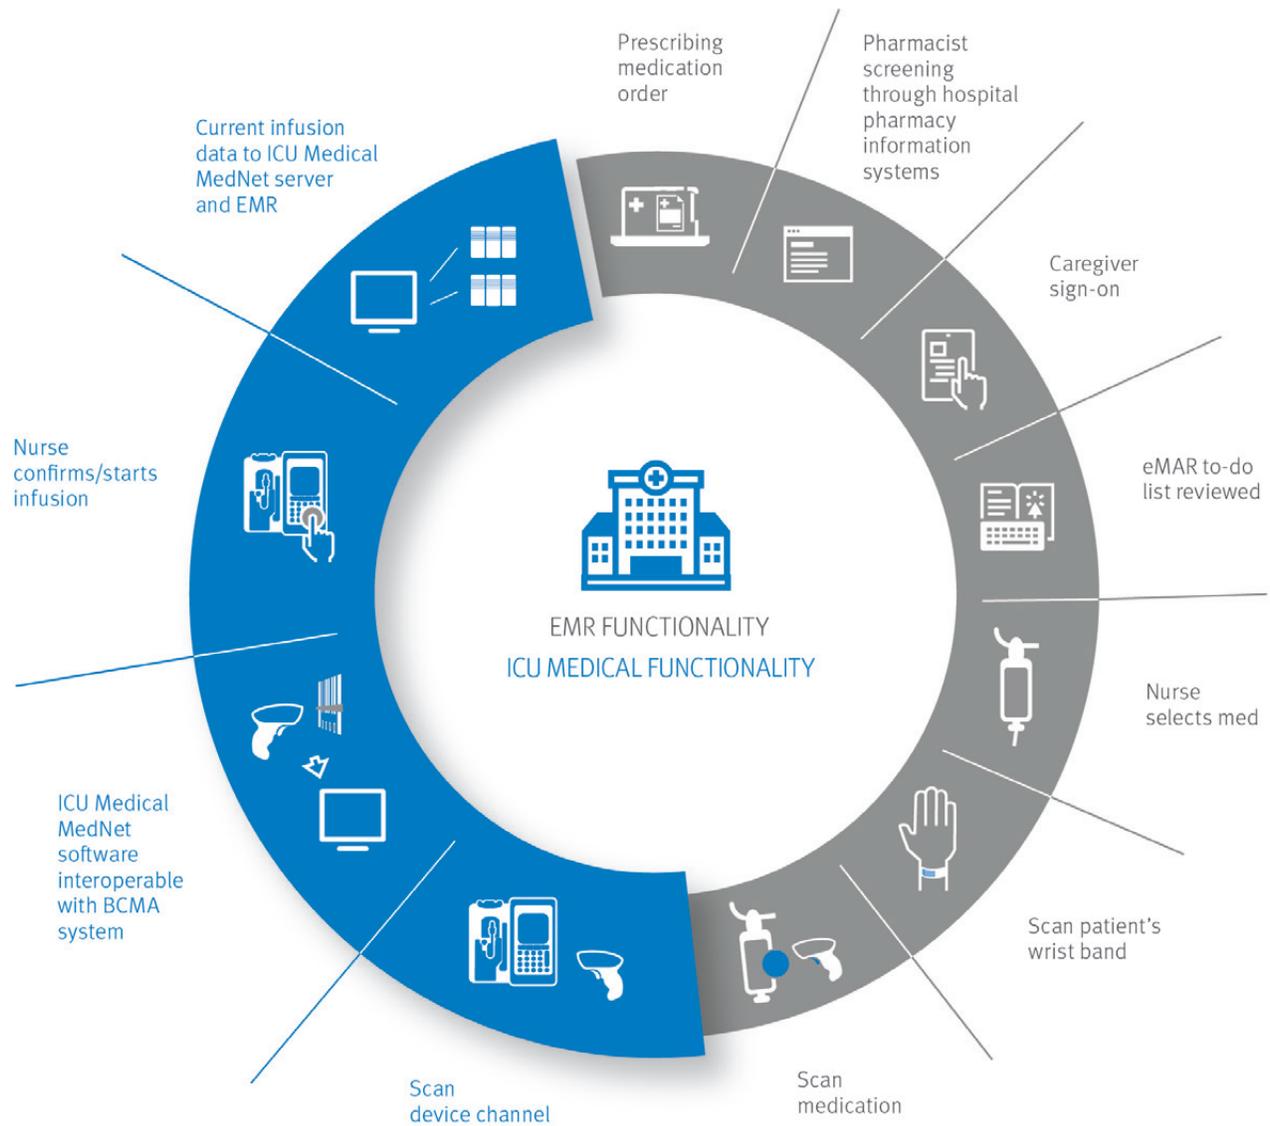


Figure 1. Clinical workflow in smart pump-EMR integrated environment

This workflow allows the physician order detail, including the fluid/medication and concentration, dose/rate, and volume to be infused (VTBI) to flow from the CPOE through the pharmacy verification process, and on to the point of care where it is automatically programmed on the pump via the barcode scanning process. The drug library alignment process is collaborative and involves the pump vendor (ICU Medical), the EMR vendor (Cerner), and the hospital pharmacy team. Depending on the degree of alignment required and the availability of resources, it typically takes three to five months and includes several rounds of testing, including connectivity and communication between the EMR system and ICU Medical infusion pumps.

Prior to the go-live date, a clinical readiness and impact assessment of IV therapy clinical nursing and pharmacy practice conducted by ICU Medical Clinical Services identifies variations in clinical practice, as well as opportunities for standardization of infusion therapy workflow.

The goal of the assessment is to increase quality of care by reducing variability in infusion therapy clinical practice. This process typically takes two to four weeks and includes a written report on the findings.

All unique ICU Medical MedNet drug library entries are tested prior to go live to ensure optimization of the integration through verification of required workflows and accuracy of clinical documentation.

Statistical Analysis



Statistical analysis was performed using Minitab® 17 and Microsoft® Excel® 2010. Decrease in the incidence of PCDEs and increase in compliant programming before and after CIDER were compared for the cohort of hospitals individually and combined using a test for two proportions. Statistical significance was determined using Fisher's exact test.

Results²



The incidence of PCDEs across the three hospitals combined decreased after CIDER by 52%, from 7.1 errors per 1000 programs to 3.3 per 1000 programs, $P < 0.001$ (Table 1). Increase in compliance with drug library was 156% between the pre- and post-integration periods for all three hospitals combined from 20% to 51%, $P < 0.001$ (Table 2). Variability in the severity of individual PCDEs also displayed a large and statistically significant reduction.

All three of these metrics improved at each hospital.

When analyzing data month by month over the study period, the reduction in PCDEs clearly pivoted around the go-live date and is sustained after integration.

Potentially Catastrophic Dosing Errors (PCDEs) Programs Pre- vs. Post-CIDER²

Potentially Catastrophic Dosing Error Rate/1000 Programs Pre- vs. Post-CIDER				
PCDE Rate per 1000 Programs				
	Pre-Integration	Post-Integration	Percent Change in PCDE Rate	Pre-Integration vs. Post-Integration PCDE Rate
FACILITY 1	9.5	2.6	-73%	p<0.001
FACILITY 2	6.8	3.6	-48%	p<0.001
FACILITY 3	5.3	3.4	-37%	p=0.08
COMBINED*	7.1	3.4	-52%**	p<0.001

*Overall rate including all three facilities

**Calculated as $[(\text{Post-CIDER PCDE rate per 1000 programs} - \text{Pre-CIDER PCDE rate per 1000 programs}) / \text{Pre-CIDER PCDE rate per 1000 programs}] \times 100$

Table 1. Pre- and post-smart pump-EMR integration—potentially catastrophic dosing errors (per 1000 programs)

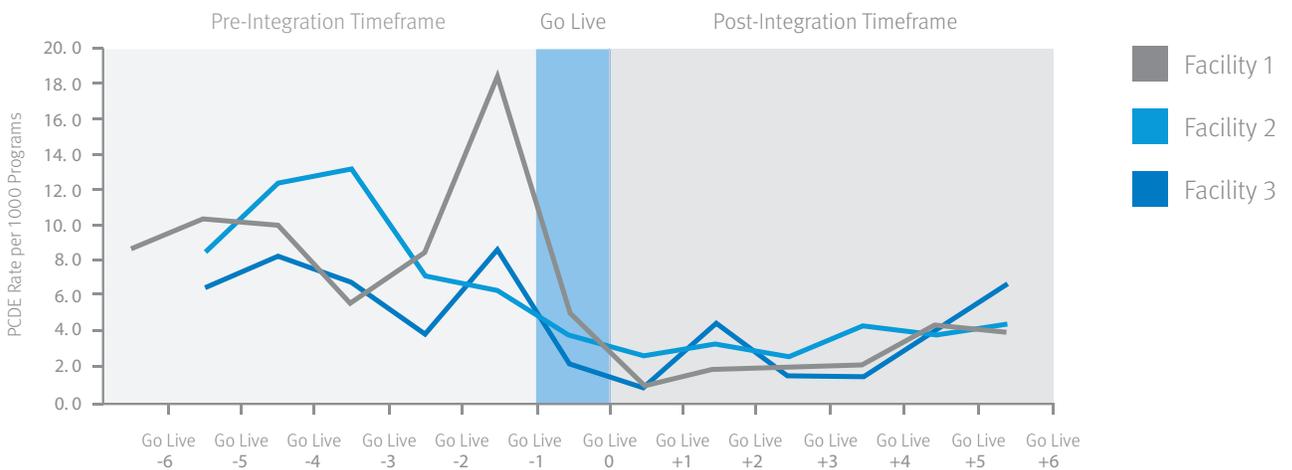


Figure 2. Pre- and post-smart pump-EMR integration—potentially catastrophic dosing errors (per 1000 programs)

ICU Medical MedNet Drug Library (DL) Compliance Pre- vs. Post-CIDER²

	Pre-Integration		Post-Integration		Pre-IVCI vs. Post-IVCI Drug Library Compliance
	Number of DL Programs	Drug Library Compliance	Number of DL Programs	Drug Library Compliance	
FACILITY 1	7,650	16.9%	24,885	51.5%	p<0.001
FACILITY 2	32,449	19.8%	111,248	51%	p<0.001
FACILITY 3	5,080	31.8%	11,927	56.2%	p<0.001
	Number of DL Programs	Drug Library Compliance	Number of DL Programs	Drug Library Compliance	Percent Change
COMBINED*	45,179	20.1%	148,060	51.4%	156%**

*Calculated as [# Combined Compliant Programs/# Combined Total Programs] x 100

**Calculated as [(Post-CIDER Combined % Compliance – Pre-CIDER Combined % Compliance)/Pre-CIDER Combined % Compliance] x 100

Table 2. Pre- and post-smart pump-EMR integration compliance with drug library

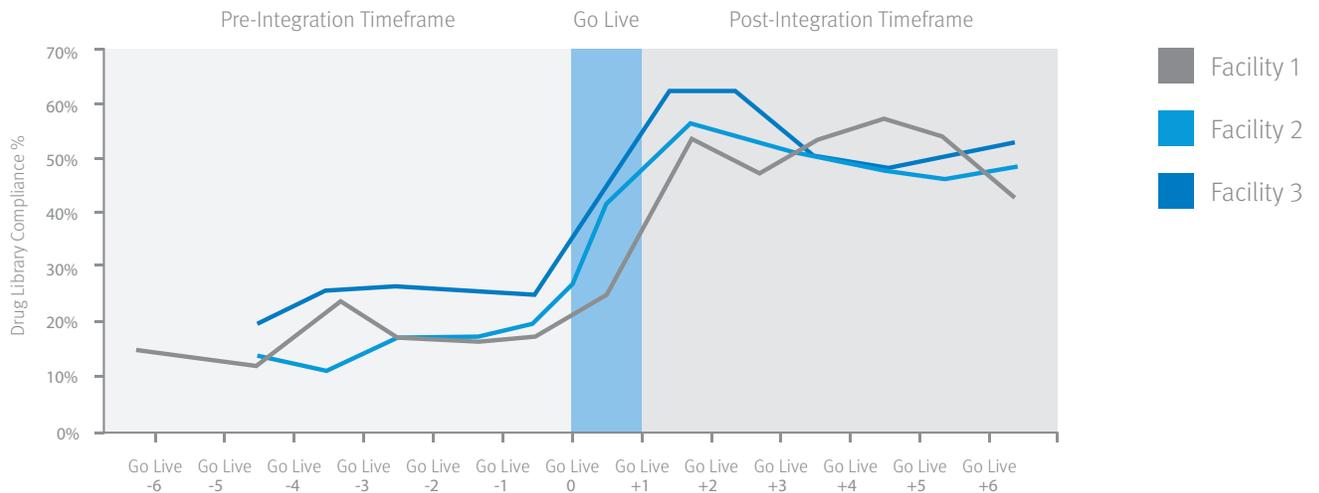


Figure 3. Pre- and post-smart pump-EMR integration compliance with drug library

PCDE Rate Variance Comparison

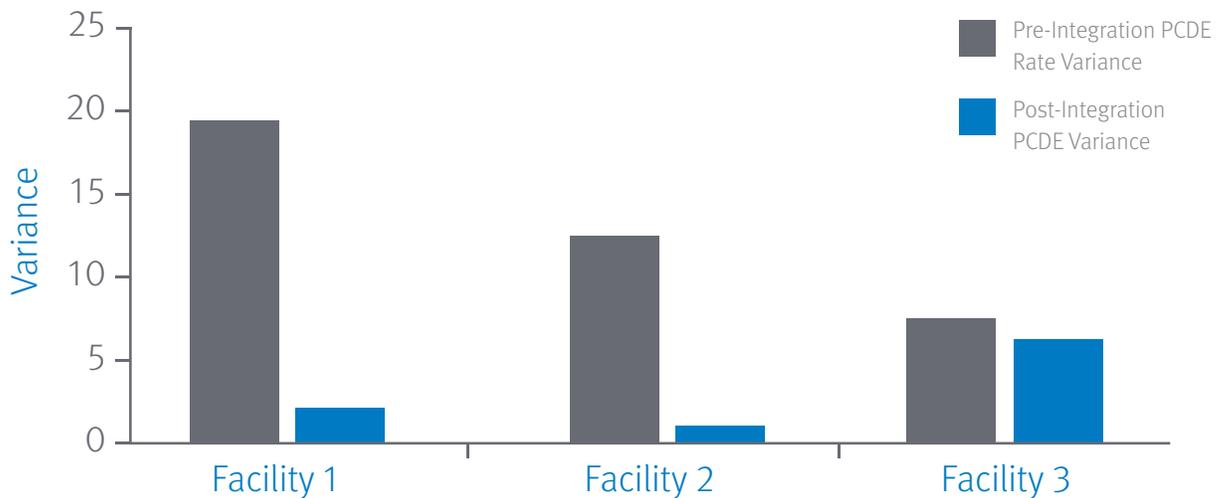


Figure 4. Pre- and post-smart pump-EMR integration—PCDE rate variance

Discussion



Our analysis of programming behavior demonstrates a significant ($p < 0.001$) and consistent decrease in the rate of potentially catastrophic programming errors after smart pump-EMR integration. In addition, our data confirms previous work from Prusch and others that integration of infusion devices with the EMR improved compliance with drug library use.^{6,7}

These improvements are equally significant and sustained in the large hospital as in the two smaller hospitals. Both the reduced range of variance of PCDEs and the narrower confidence intervals in the post-integration data demonstrate that variability in programming is greatly reduced after integration. Reducing variability in practice is an objective for improving the quality of healthcare, as it has also been in other industries.

The safety gains of smart pump-EMR integration address historical infusion risks, including differences between hospitals in how medications are ordered, processed in a hospital pharmacy, and ultimately delivered to a patient. For example, a physician may order a medication in a certain concentration, but the pharmacy may fill the prescription at a different concentration for any variety of reasons, (e.g., availability and cost). If the nurse fails to notice the difference in the concentrations, an incorrect infusion may be manually programmed into the pump. The barcode scanning process at the point of care provides “five rights” verification and mitigates this risk. Work-arounds and idiosyncrasies of workflow in hospitals, units, or practitioners also play a role in practice variation. Nurses routinely reduce VTBI by 50–100 mL or shorten the duration of the infusion to only one to two hours to encourage more frequent assessment of the infusion. Manual admixing of medications still occurs at the unit level by nurses, as does syringe delivery of unit doses.

Both the reduced range of variance of PCDEs and the narrower confidence intervals in the post-integration data demonstrate that variability in programming is greatly reduced after integration.

With the implementation of smart pump technology, hospitals are able to better define safety parameters for IV medications. Analysis of the data can provide insight into current processes and actionable items to be included in CQI initiatives.

Sustainability must be carefully considered. Because manual programming should remain an option and is occasionally necessary, end-user involvement in the development of process improvements will be critical to successful clinical adoption of the integration.

There are several reasons why CIDER did not improve compliance beyond the mid-fifties with use of the drug library. There were fluids and medications that were out of scope, such as boluses, blood products, and banana bags. Programming of infusions during emergencies, such as code blue and rapid response calls, was often done manually. In addition, our methodology counted manual titrations to a noncompliant infusion as separate noncompliant events, reducing the overall compliance numbers. Lastly, when use of the drug library is optional for manual programming, it is imperative that clinical leadership drive and communicate the expectation that the drug library be used for all infusions. In our study, there was an integration learning curve for both leadership and frontline providers, which is not atypical in adoption of new technologies.

There are several limitations in this data set and its interpretation. This study was not a prospective, randomized controlled trial of patient outcomes but a pre- and post-intervention design, which is susceptible to bias.

We were unable to determine programming errors for programming episodes where the drug library was not selected, as these noncompliant data entries could not be recovered in the data stream. Thus we were only able to demonstrate that CIDER reduced potentially catastrophic programming errors in the subset of events that was compliant with use of the drug library. Although this proportion of programming episodes increased significantly after integration and the proportion of catastrophic errors in this subset was reduced, we cannot conclude the overall number of catastrophic errors was reduced since we had no visibility to the noncompliant proportion of programming events either before or after integration.

We chose to include ISMP high-alert drugs in the medication set most likely to cause harm and affect the NCC MERP classification. However, there are intravenous medications not included in this set that may cause harm, and not every programming error with a high-alert drug will lead to harm.

In conclusion, this study adds to the body of evidence that clinical integration of the EMR with infusion devices may offer patient safety advantages and simplify provider workflow. Additional longitudinal studies are needed to confirm these results.

Keywords

- Medication safety
- Adverse drug events
- Infusion pump
- Smart pump-EMR integration
- Human factors



References

1. Ohashi K, Dalleur O, Dykes PC, et al. Benefits and risks of using smart pumps to reduce medication error rates: a systematic review. *Drug Saf.* 2014;37(12):1011-1020.
2. ICU Medical, Inc. Data on file. Analysis of ICU Medical MedNet data. 2014.
3. Hess P. Smart pump/EMR integration: What are my best options? May 2015 Performance Report. ©2015. KLAS Enterprises, LLC. All rights reserved. Available at www.KLASresearch.com.
4. The National Coordinating Council for Medication Error Reporting and Prevention (NCC MERP). NCC MERP Index for Categorizing Medication Errors. Adopted July 16, 1996. Revised February 20, 2001. Available at <http://www.nccmerp.org/sites/default/files/indexColor2001-06-12.pdf>. Accessed January 23, 2017.
5. Institute for Safe Medication Practices (ISMP). ISMP list of high-alert medication in acute care settings [web page]. Created 2014. Available at <https://www.ismp.org/Tools/highalertmedications.pdf>. Accessed May 16, 2016.
6. Prusch AE, Suess TM, Paoletti RD, et al. Integrating technology to improve medication administration. *Am J Health Syst Pharm.* 2011;68(9):835-842.
7. Pettus DC, VanderVeen T. Worth the effort? Closed-loop infusion pump integration with the EMR. *Biomed Instrum Technol.* 2013;47(6):467-477.

About the Authors

Valerie King, MS, BSN, is a Senior Clinical Consultant for ICU Medical. She previously held leadership positions in acute care, provided consulting services for implantable technologies, and served as Senior Clinical Care Coordinator and Marketing Director for a large physician practice.

Douglas Hum, RPh, is a Pharmacy Consultant for ICU Medical. Prior to joining ICU Medical, he served as Pharmacy Operations Manager at United Hospital in Saint Paul, MN, Pharmacy Director at Medica Health Plan, and Clinical Director of Clinical Services/Managed Care Plans for CVS Caremark.

Don Kendzierski, Pharm D., is a Pharmacy Consultant and Analytics Program Coordinator for ICU Medical and a Six Sigma Black Belt. Prior to joining ICU Medical, he held pharmacy practice leadership positions for academic medical centers and the Department of Veterans Affairs.

Candida Arvelo, MBA, BSN, was the Director of Clinical Services for ICU Medical. She previously served as a Department Clinical Director at HCA Houston for more than 10 years.

Frank Overdyk, MSEE, MD, previously served as the Medical Director, Devices at ICU Medical, a Pfizer company. Dr. Overdyk currently serves on the anesthesiology staff at Roper St. Francis Health System in South Carolina.

