



Clave™ Neutron™

Needlefree Neutral Displacement Connector

A needlefree neutral displacement connector featuring ICU Medical's clinically-differentiated Clave infection control technology with a bidirectional valve designed to prevent blood reflux and help minimise occlusions

icumedical
human connections

The Clave Neutron needlefree neutral displacement connector is designed to reduce reflux to help

Minimise Occlusions

Maintaining catheter patency and minimising occlusions can be important steps in your efforts to enhance patient safety and help reduce costs.

Despite your efforts, central line occlusions—which are frequently caused by blood reflux—remain a significant issue that can result in delays in critical patient care, increased risk of infection, and increased healthcare costs. That's why reducing the risk of catheter occlusions may help you decrease the need for expensive clotting agents, such as t-PA, and reduce the clinical costs associated with managing catheter occlusions.

Neutron's innovative anti-reflux technology helps stop occlusions before they start while providing a safe and effective microbial barrier.

Our Neutron needlefree neutral displacement connector is designed to prevent the four known causes of displacement associated with needlefree connectors: connection or disconnection of a luer, syringe plunger compression, patient vascular pressure changes (i.e., coughing or sneezing), and IV solution container run-dry, which may cause multiple forms of reflux into a catheter.¹

The Clave Neutron also utilises ICU Medical's Clave needlefree connector technology, which is proven to minimise contamination and help you lower the risk of catheter-related bloodstream infections (CRBSI)^{2,3,4,5,6,7}.

Clave Neutron
May Help You Reduce
Catheter Occlusions by

50%⁸



Helping reduce catheter occlusions with the Clave Neutron needlefree neutral displacement connector may provide real-time clinical benefits.



Avoid Delays in Critical Patient Care

Clave Neutron may help avoid delays in therapy of critical intravenous medications (e.g., antibiotics and oncolytics), nutritional support, and blood products.



Avoid Patient Discomfort and Pain

Clave Neutron may help avoid patient discomfort and pain caused by unnecessary needlesticks, catheter restarts, and manipulation of the IV site.



Avoid Unnecessary Costs

Clave Neutron may help minimise unnecessary costs that add up when treating an occlusion.



Help Reduce Risk of Infection


Clave Neutron may help reduce the risk of infection by preventing thrombosis and minimising IV line manipulation.

Designed to prevent multiple causes of reflux into a catheter

Reflux of blood into the catheter has been shown to contribute to biofilm formation and catheter occlusion.

Internal Causes

- › Patient Vascular Pressure Changes Caused by:
 - › Coughing
 - › Sneezing
 - › Movement
 - › Crying

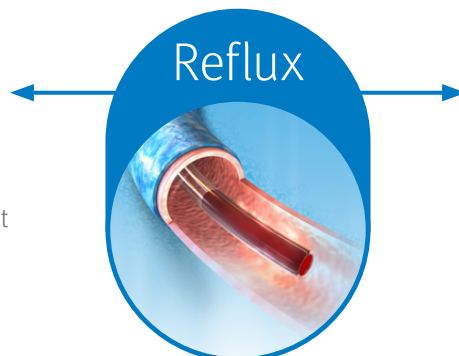


External Causes

- › Connection and Disconnection of a Luer
- › IV Bag Running Dry or an Infusion Pump Stopping
- › Syringe Plunger Rebound


Advanced Anti-Reflux Technology

Because of an innovative design incorporating a proprietary, bi-directional silicone valve and bellows feature to help prevent reflux, Clave Neutron helps maintain catheter patency during the times traditional connectors have been shown to occlude most often.



Valve During Aspiration

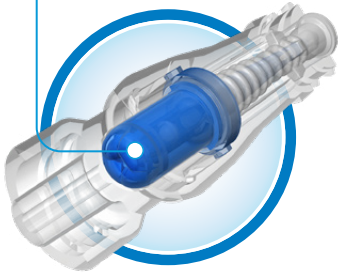

Valve During Infusion

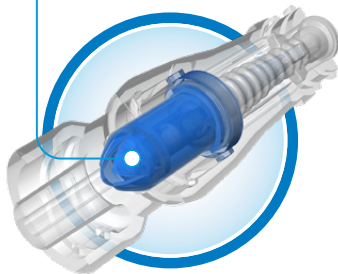

Valve With No Fluid Flow

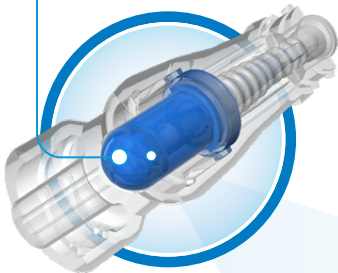

Valve During Reflux Challenge

Unlike other anti-reflux valves, Neutron's proprietary technology provides the unique ability to absorb and physically compensate for pressure variations that typically result in blood reflux into a catheter.



Clinically-differentiated Infection Control Technology

Proven to Minimise Bacterial Contamination^{2,3,4,6,7}

Clave Neutron can help your efforts to reduce bloodstream infections by minimising entry points for bacteria and maximising the effectiveness of every flush.



Silicone Seal and Internal Cannula Minimises Point of Entry for Bacteria

Specifically designed to minimise contact between the connector's external surface and the internal fluid path upon luer activation, Clave Neutron needlefree IV connectors minimise entry points for bacteria. Several studies have attributed this feature to a reduction in bacterial contaminants passed through the connector.^{2,3,4,9}

Split Septum

Clave Neutron's normally closed, swabbable split septum design is a preferred feature for needlefree connectors.¹⁰

Straight Fluid Path

Clave Neutron's straight fluid path allows for efficient clearing of medications, blood, and blood residual with low flush volumes.^{11,12}

Minimal Residual Volume

Clave Neutron's minimal residual volume allows for lower flush volumes.

Clear Housing


A clear housing lets you see whether you have completely flushed the connector after blood draws or administration.

Add a Splash of Color For Quick and Easy Line Identification.

Customise Neutron with a variety of color-coded rings to help you improve IV line management and avoid medication mix-ups.

Color-coded needlefree IV connector rings designed to help reinforce your facilities line-identification initiatives:

- › Enhance patient safety and reduce the possibility of medication errors
- › Quickly access the proper infusion port in emergency situations
- › Improve connector change interval compliance with better needlefree connector identification

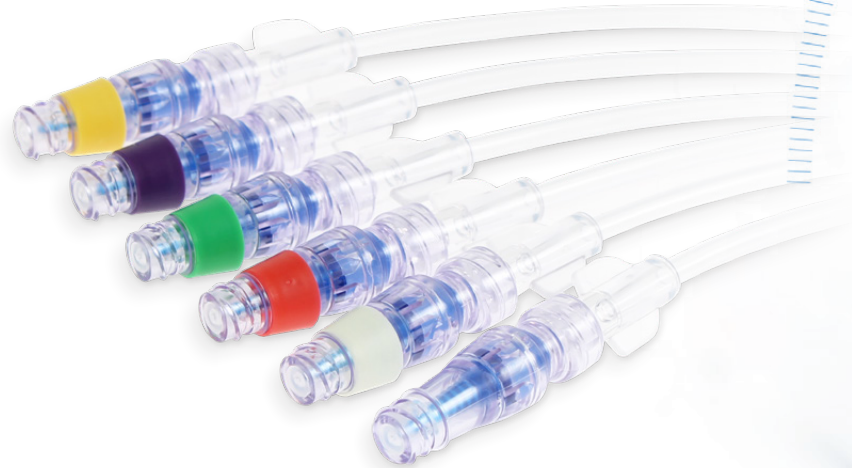

To learn more about ICU Medical's Clave Neutron neutral displacement connector, please call 1300 428 652 (Aus) or 0800 629 637 (New Zealand)

Technical Specifications

| | |
|-----------------------------|---------------------|
| Residual Volume | 0.1 mL |
| Flow Rate at Gravity | 100 mL/minute |
| Blood Compatibility | Yes |
| MRI Compatibility | No Metal Components |
| High Pressure Compatibility | 10 mL/second |

Drug Compatibility

| | |
|--------------|-----|
| Alcohol | Yes |
| Lipids | Yes |
| Chemotherapy | Yes |



Neutron's saline flush option is designed to help you reduce risks, cost, and time associated with Heparin use.

1. ICU Medical Clave Neutron 510(k) K100434, June 24, 2010
2. Ryder M, RN, PhD. Comparison of Bacterial Transfer and Biofilm Formation on Intraluminal Catheter Surfaces Among Twenty Connectors in a Clinically Simulated In Vitro Model. Presented at World Congress Vascular Access (WoCova) 2018.
3. JD Brown, HA Moss, TSJ Elliott. The potential for catheter microbial contamination from a needleless connector. J Hosp Infect. 1997; 36:181-189.
4. Yebenes J, Delgado M, Sauca G, Serra-Prat M, Solsona M, Almirall J, et al. Efficacy of three different valve systems of needlefree closed connectors in avoiding access of microorganisms to endovascular catheters after incorrect handling. Crit Care Med 2008;36: 2558-2561.
5. Moore C, RN, MBA, CIC. Maintained Low Rate of Catheter-Related Bloodstream Infections (CR-BSIs) After Discontinuation of a Luer Access Device (LAD) at an Academic Medical Center. Poster presented at the annual Association for Professionals in Infection Control and Epidemiology (APIC) Conference 2010, Abstract 4-028.
6. Data on file at ICU Medical. Microbial Ingress Study on Clave Technology Study commissioned by ICU and conducted by Nelson Laboratories, 2008.
7. Data on file at ICU Medical. Microbial Ingress Study on Neutron Connector. Study commissioned by ICU and conducted by Nelson Laboratories, 2017.
8. Observational In-Vivo Evaluation of the Neutron™ Needlefree Catheter Patency Device and its Effects on Catheter Occlusions in a Home Care Setting, 2011
9. Bouza E, Munoz P, Lopez-Rodriguez J, et al. A needleless closed system device (Clave™) protects from intravascular catheter tip and hub colonization: a prospective randomized study. J Hosp Infect. 2003; 54:279-287.
10. Guidelines for the Prevention of Intravascular Catheter-Related Bloodstream Infections, 2011 (Updated Recommendations July 2017)
11. Breznock EM, DVM, PhD, Diplomate ACVS, Sylvia CJ, DVM, MS, BioSurg, Inc. The in vivo evaluation of the flushing efficiency of different designs of clear needlefree connectors, March 2011.
12. Data on file at ICU Medical. Low Volume Flush Characteristics of Unique Needlefree Connectors M1-1223 Rev. 1.