

Product Reference Guide

Grifols Fleboflex® Container IV Solutions

0.9% Sodium Chloride Injection, USP, in Fleboflex Container

Instructions for Use

1. Remove Overwrap



› The overwrap serves as a moisture barrier. It is intended to limit evaporative moisture loss from the primary solution container.
› The overwrap is opened by pulling apart the two sheets of the overwrap.



› To remove the overwrap, peel off one sheet by the corner while holding the other sheet at one end and carefully removing the solution container.

Note: The overwrap should not be removed until product is to be used.

2. Inspect Container

› Visually inspect the container for particulate matter and discoloration.
› Check for minute leaks by squeezing inner container firmly.
› If leaks are found, discard solution as sterility may be impaired.
› If the outlet port protector is damaged, detached, or not present, discard container as the solution path sterility may be compromised.


Note: Do not administer unless the solution is clear and seal is intact.

3. Add Medication



› Prepare medication site.
› Using a syringe with a 19 to 22 gauge needle, securely hold the container. Insert the needle through the center of the medication port and inject.

Note: Check the compatibility of the additives with sodium chloride 0.9% before adding a medication.

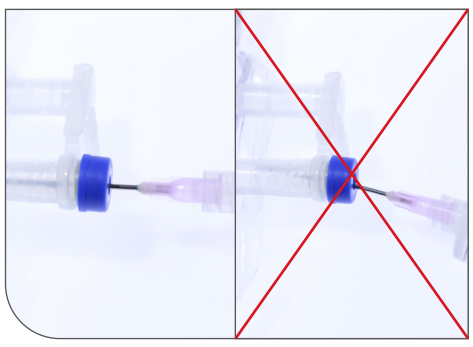

› Insert the needle perpendicular to the point of addition.

4. Attach Administration Set



› Suspend the container from eyelet support and remove the protector from the outlet port at the bottom of the container.



› Hold the container properly and attach the administration set.

Attach Administration Set (Continued)



› While advancing through the tube, a slight resistance will gradually appear.

Note: To ensure proper connection and prevent leakage, push the administration set using a rotary motion up to the shoulder of the spike.




› Reference the image to know if the administration set is correctly attached.

5. Use Non-vented Administration Sets



› The Fleboflex container has been designed to work without venting. No air is required to withdraw the solution. Air entering through the administration set could slow or even stop the infusion due to air bubbles.

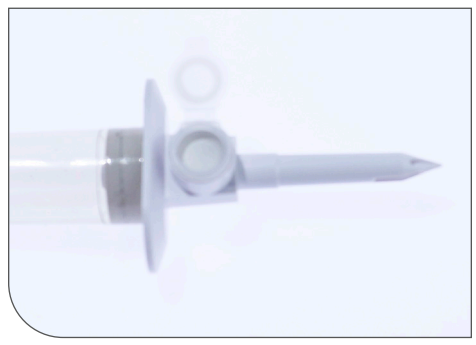

› Administration sets should come without air venting. If vented administration sets are used, be sure air venting inlet remains closed during the infusion.

Note: After opening the container, the contents should be used immediately and should not be stored for a subsequent infusion. Do not reconnect any partially used containers. Discard any unused portion.

Note: Do not connect flexible plastic containers in a series to avoid air embolism due to possible residual air in the primary container. Use of a vented intravenous administration set with the vent in the open position could result in air embolism. Vented intravenous administration sets with the vent in the open position should not be used with flexible plastic containers.

*Manufactured by Laboratorios Grifols S.A. and distributed by ICU Medical Sales, Inc.
Fleboflex® is a registered trademark owned by Grifols Worldwide Operations Limited.

GRIFOLS

Manufactured for ICU Medical by:

Laboratorios Grifols S.A. Calle Marte nº4
Polígono Industrial Los Llanos
30565 Las Torres de Cotillas, Murcia
SPAIN
www.grifols.com

© 2026 Grifols All rights reserved US-FBX-2600015

℞ Only For safe and proper use, refer to the Instructions for Use.

Distributed by:

icumedical
human connections

800.824.7890 | www.icumed.com

© 2026 ICU Medical Inc. | C26-4967